MIDMARK®

Installation/Operation Instructions

9A273001 KNEE CRUTCH ASSEMBLY

KIT COMPONENTS

Part Number	Description	Qty.
9A273001	Knee Crutch Assy.	1
• 029-1842-00	Knee Crutch Assy.	1 pair
• 029-0613-00	Clamp Assy.	1 pair
• 003-1039-00	I / O Instructions	1

REQUIRED TOOLS

None

INTRODUCTION

To support knee and legs for pelvic examination.

WARNING

Must be mounted only on Seat rail of exam table. Must be removed or rotated clear of moving parts before positioning table. Do not use simultaneously with 9A21300X, Caster Base Assy. Always support patient's extremity when repositioning Knee Crutch.

INSTALLATION (1)

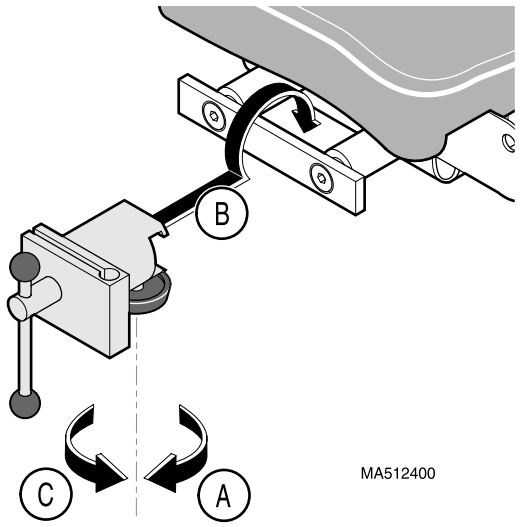

A. Loosen handle on Rail Mount Weldment.

WARNING

Handle that secures Rail Mount must be positioned below Side Rail so lip on Rail Mount hooks over top of Side Rail.

B. Hook Rail Mount over or slide it onto Side Rail.

C. Tighten handle.

INSTALLATION (2)

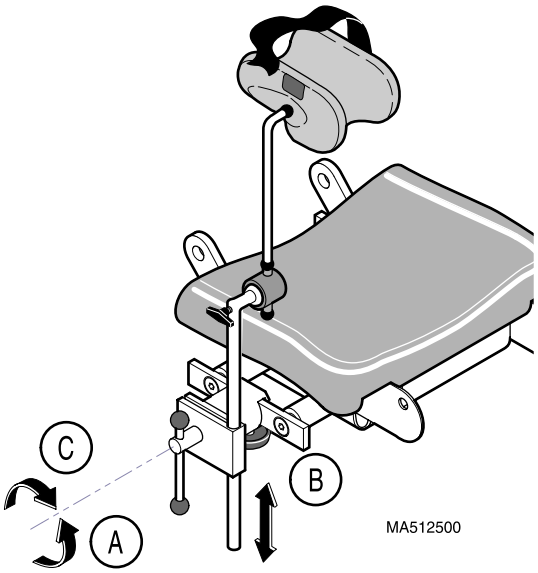

NOTE

The Assembly contains a Knee Crutch for patient's *right* and *left* side. Assure correct positioning when installing.

A. Loosen handle.

B. Insert Mounting Rod of Knee Crutch to desire height.

C. Tighten handle.

INSTALLATION (3)

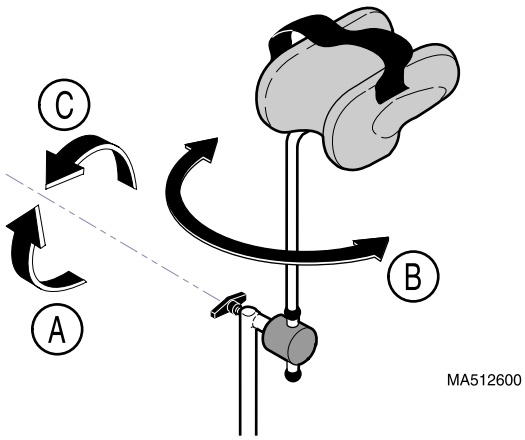

A. Loosen handle.

B. Rotate Knee Crutch to desired position.

C. Tighten handle.

NOTE

Triangle velcro strip on bottom of each Knee Crutch is for attaching restraint straps for storage when not in use.

© Midmark Corporation - 1999